



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alztal-Alpakas/Hermann Gröbner
Feldkirchner Str. 1
83308 Trostberg Germany

Date: 07/20/17

Test No: 945366


Animal and Sample Description

Animal Name: JLA Luca
Breed: Alpaca(Huacaya)
Sex: Male
Color: Lt Fawn

Animal ID: 276093400557509
Sample Location: Side (L)
Sample Date: 05/10/17
Age: 06/19/16

Laboratory Data

Mean Fiber Diameter:	16.0 microns	Fibers Greater Than 30 microns:	0.5 %
Standard Deviation:	3.5 microns	Comfort Factor:	99.5 %
Coefficient of Variation:	21.9 %	Mean Curvature:	60.2 deg/mm
Spin Fineness:	15.6 microns	SD Curvature:	34.0 deg/mm

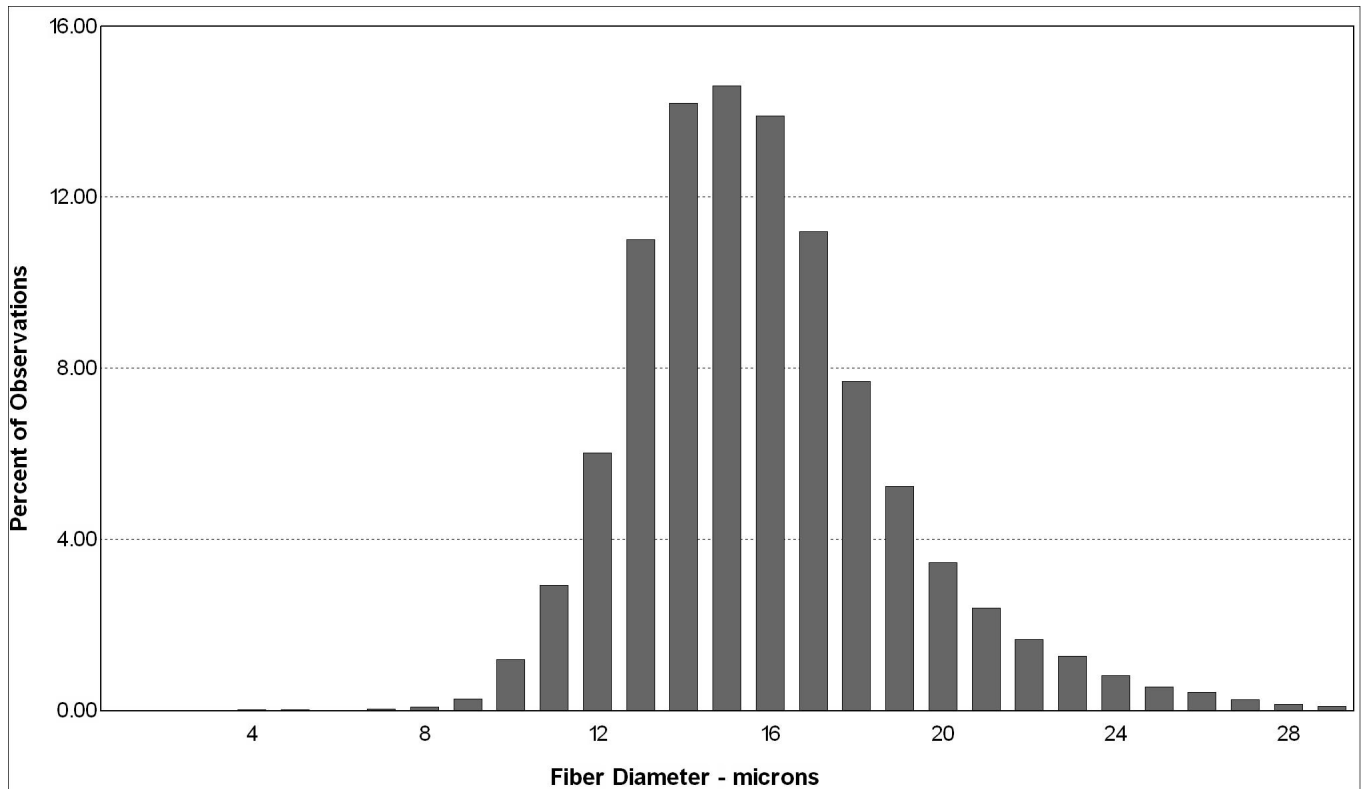

This Test Performed According to I.W.T.O Method 47