



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100) Micron Test Report

Alztal-Alpakas/Hermann Gröbner
Feldkirchner Str. 1
83308 Trostberg Germany

Date: 07/20/17

Test No: 945367


Animal and Sample Description

Animal Name: ATA Appy Shakun
Breed: Alpaca(Huacaya)
Sex: Male
Color: Appaloosa

Animal ID: 276093400560084
Sample Location: Side (L)
Sample Date: 05/10/17
Age: 07/27/15

Laboratory Data

Mean Fiber Diameter:	16.2 microns	Fibers Greater Than 30 microns:	0.7 %
Standard Deviation:	3.8 microns	Comfort Factor:	99.3 %
Coefficient of Variation:	23.4 %	Mean Curvature:	48.8 deg/mm
Spin Fineness:	16.1 microns	SD Curvature:	30.2 deg/mm

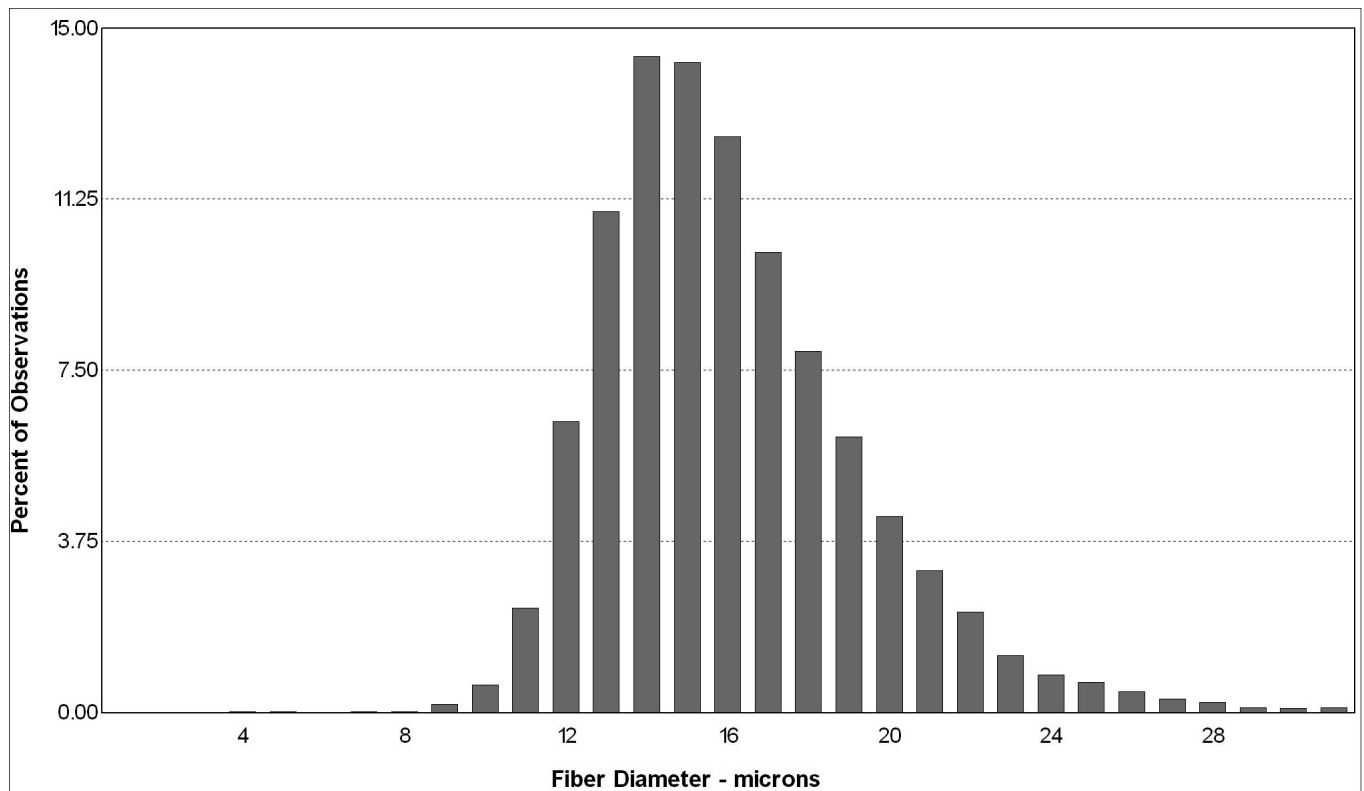

This Test Performed According to I.W.T.O Method 47